

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.**

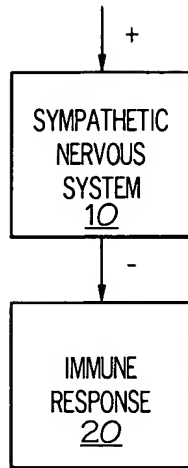


FIG. 1

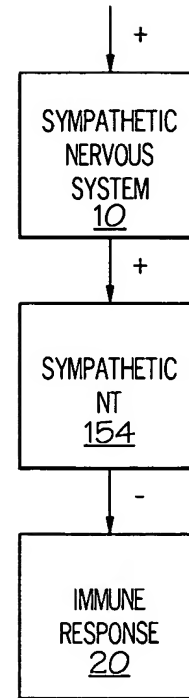


FIG. 3

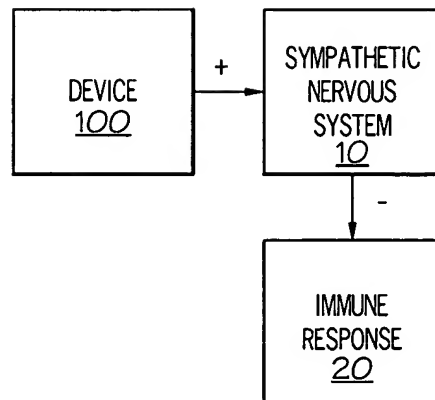


FIG. 4

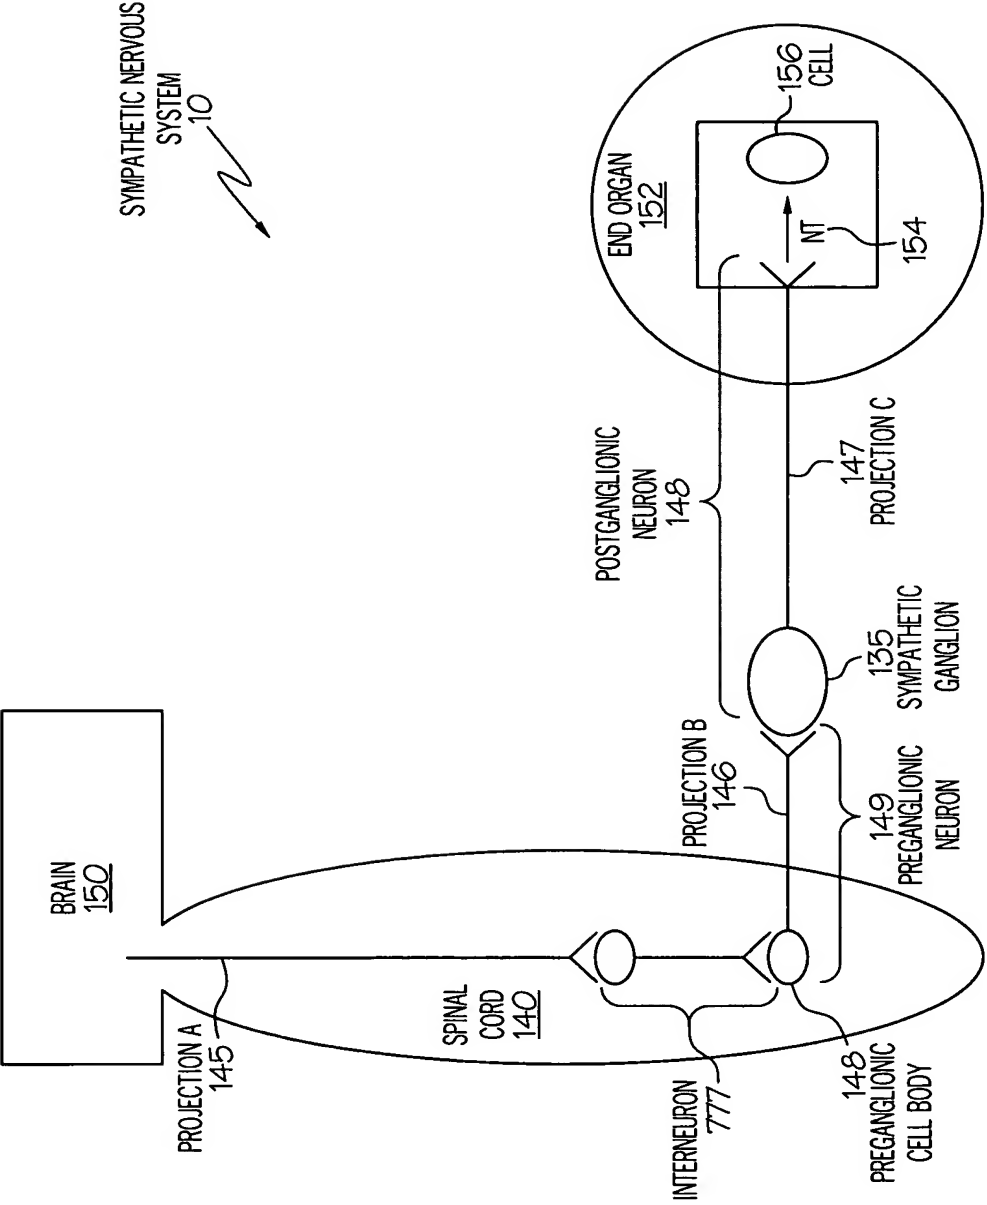


FIG. 2

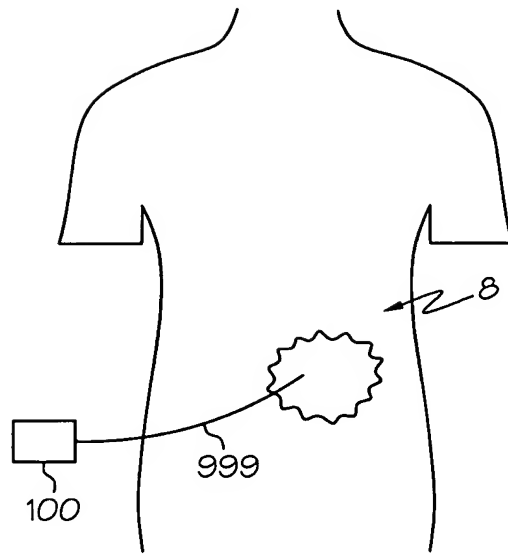


FIG. 5A

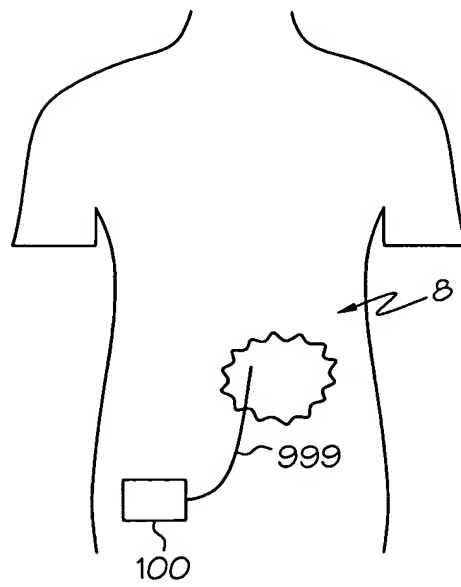


FIG. 5B

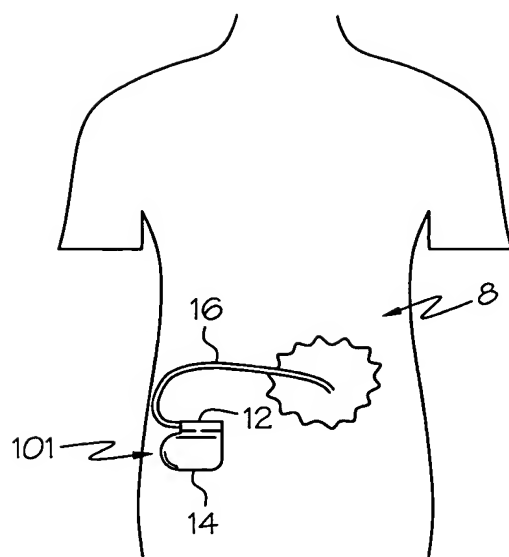


FIG. 6A

IMPLANT SYSTEM COMPONENTS

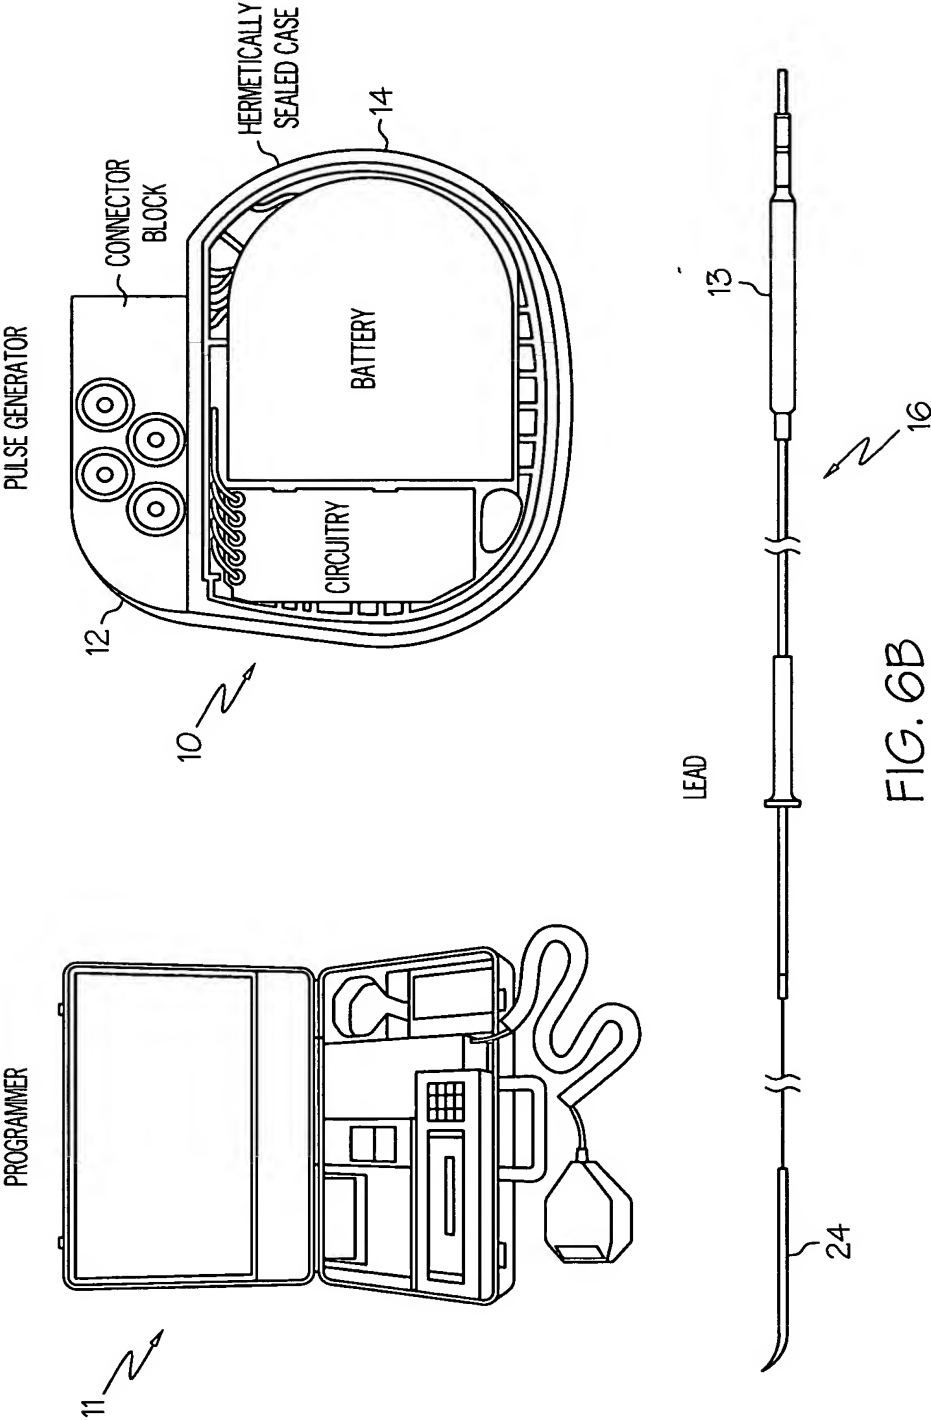


FIG. 6B

IMPLANT HARDWARE

IMPLANTABLE NEUROSTIMULATOR:	
MEDTRONIC ITREL3 (MODEL 7425G)	
NEUROMUSCULAR LEADS (2):	
MEDTRONIC MODEL 4351	
STIMULATION PARAMETERS	
AMPLITUDE:	5 milliamps
PULSE WIDTH	330 μ sec
RATE:	14Hz
CYCLE ON TIME:	0.1 sec
CYCLE OFF TIME:	5.0 sec

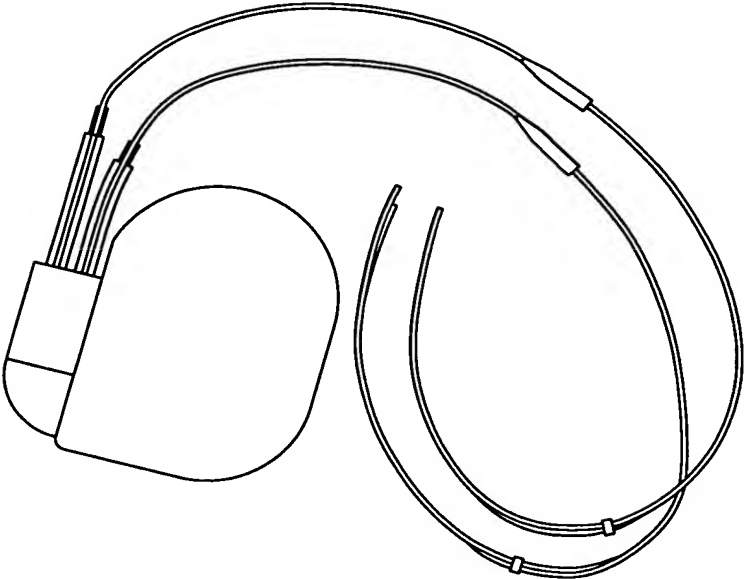
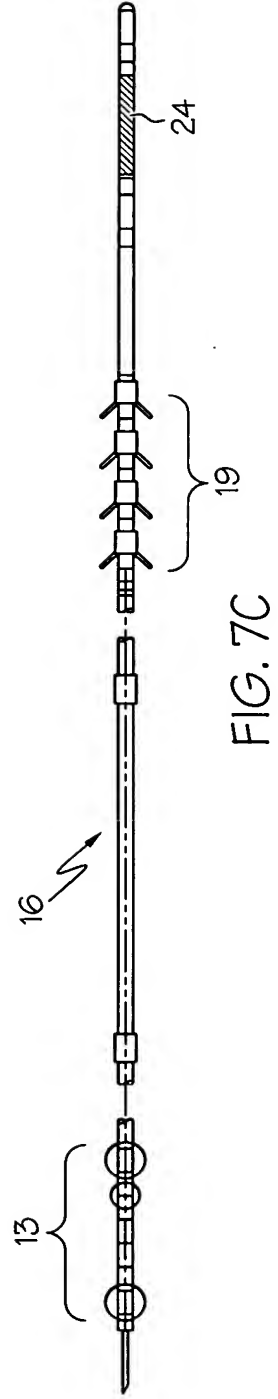
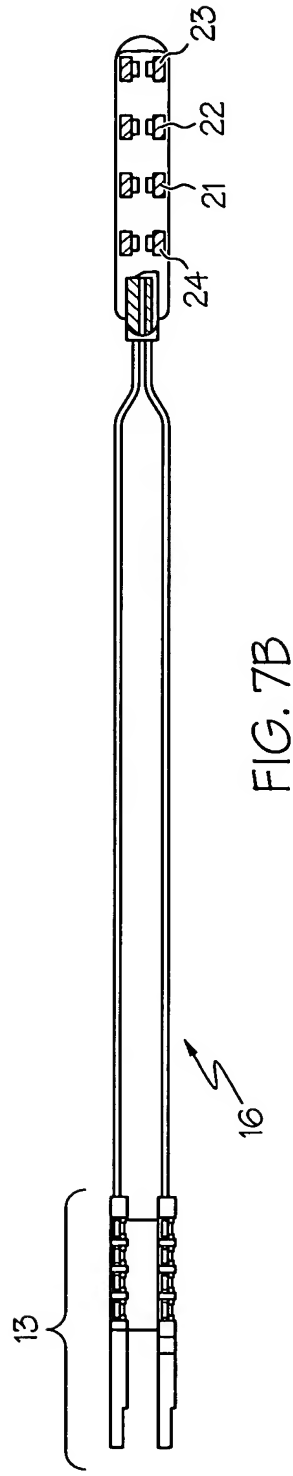
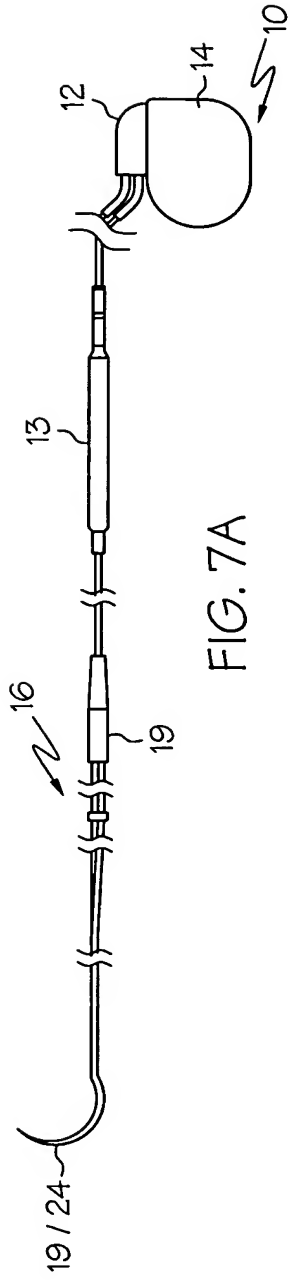


FIG. 6C



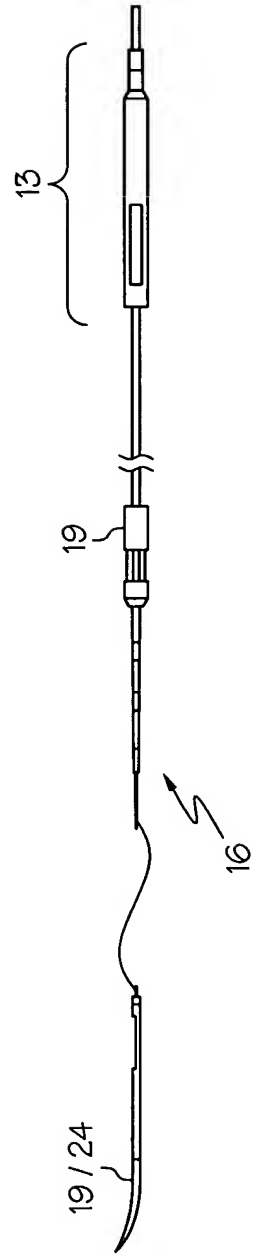


FIG. 7D

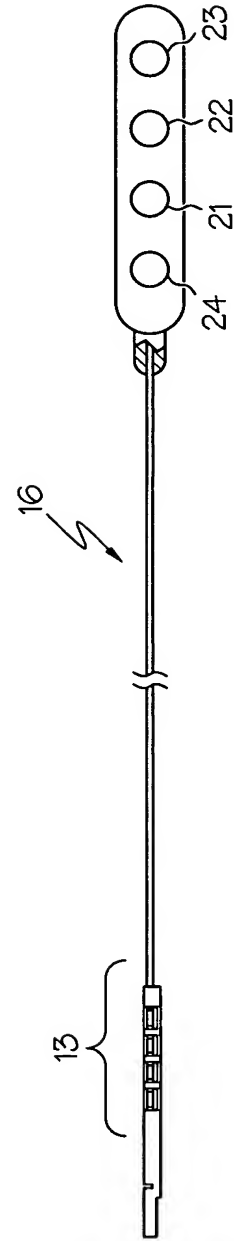


FIG. 7E

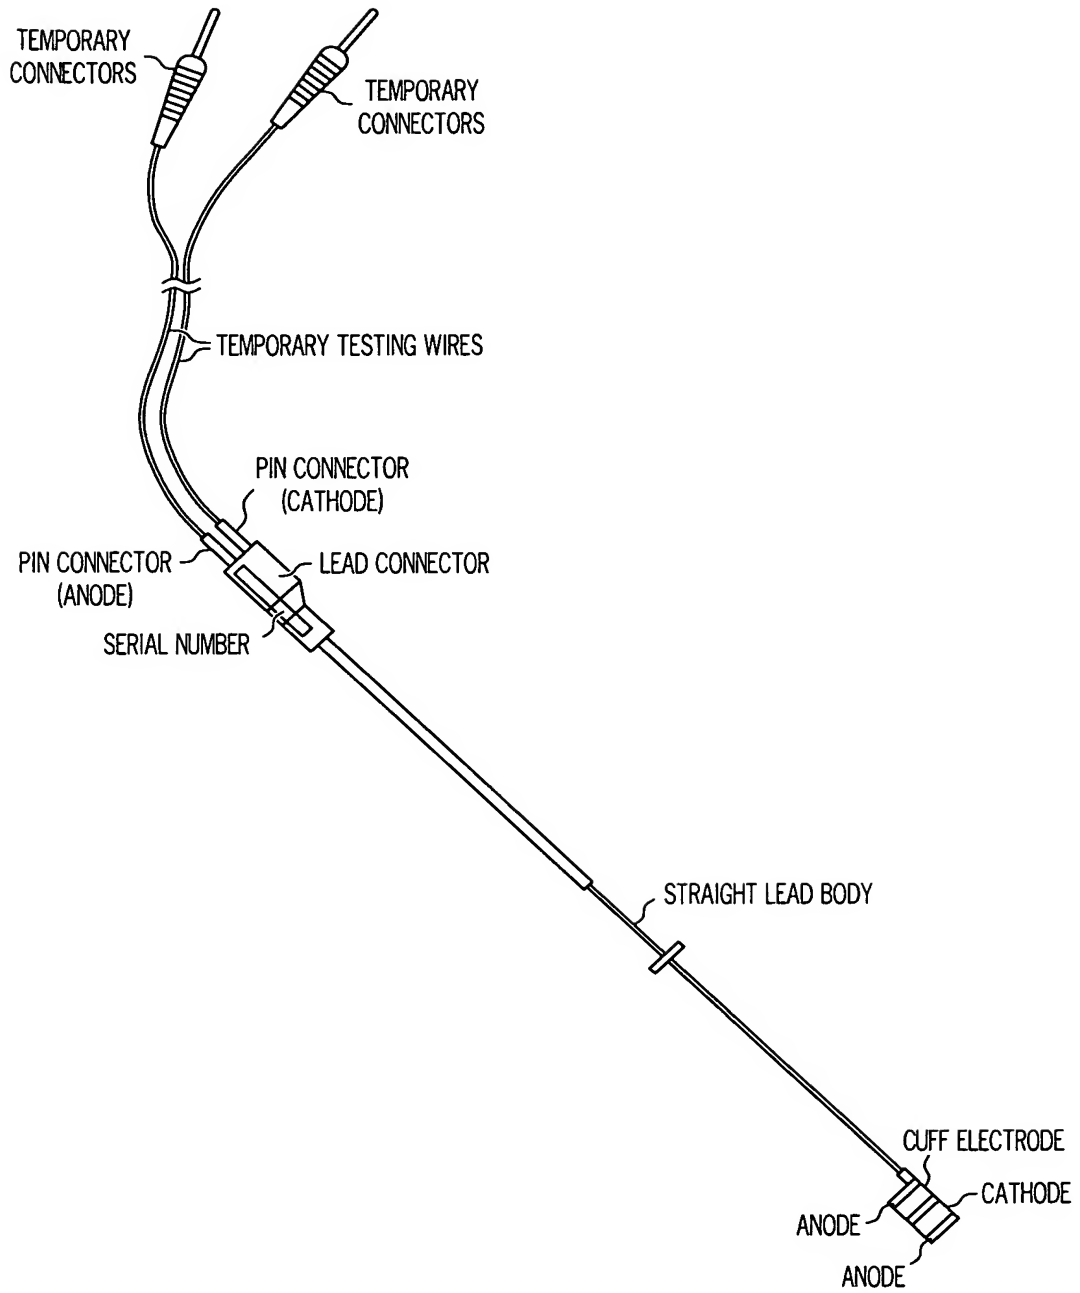


FIG. 7F

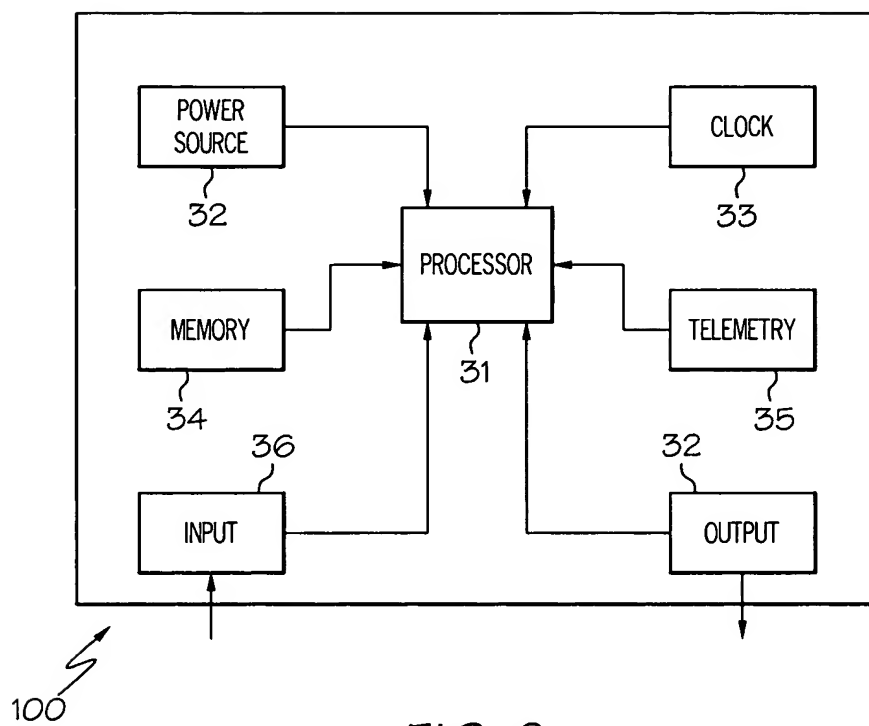


FIG. 8

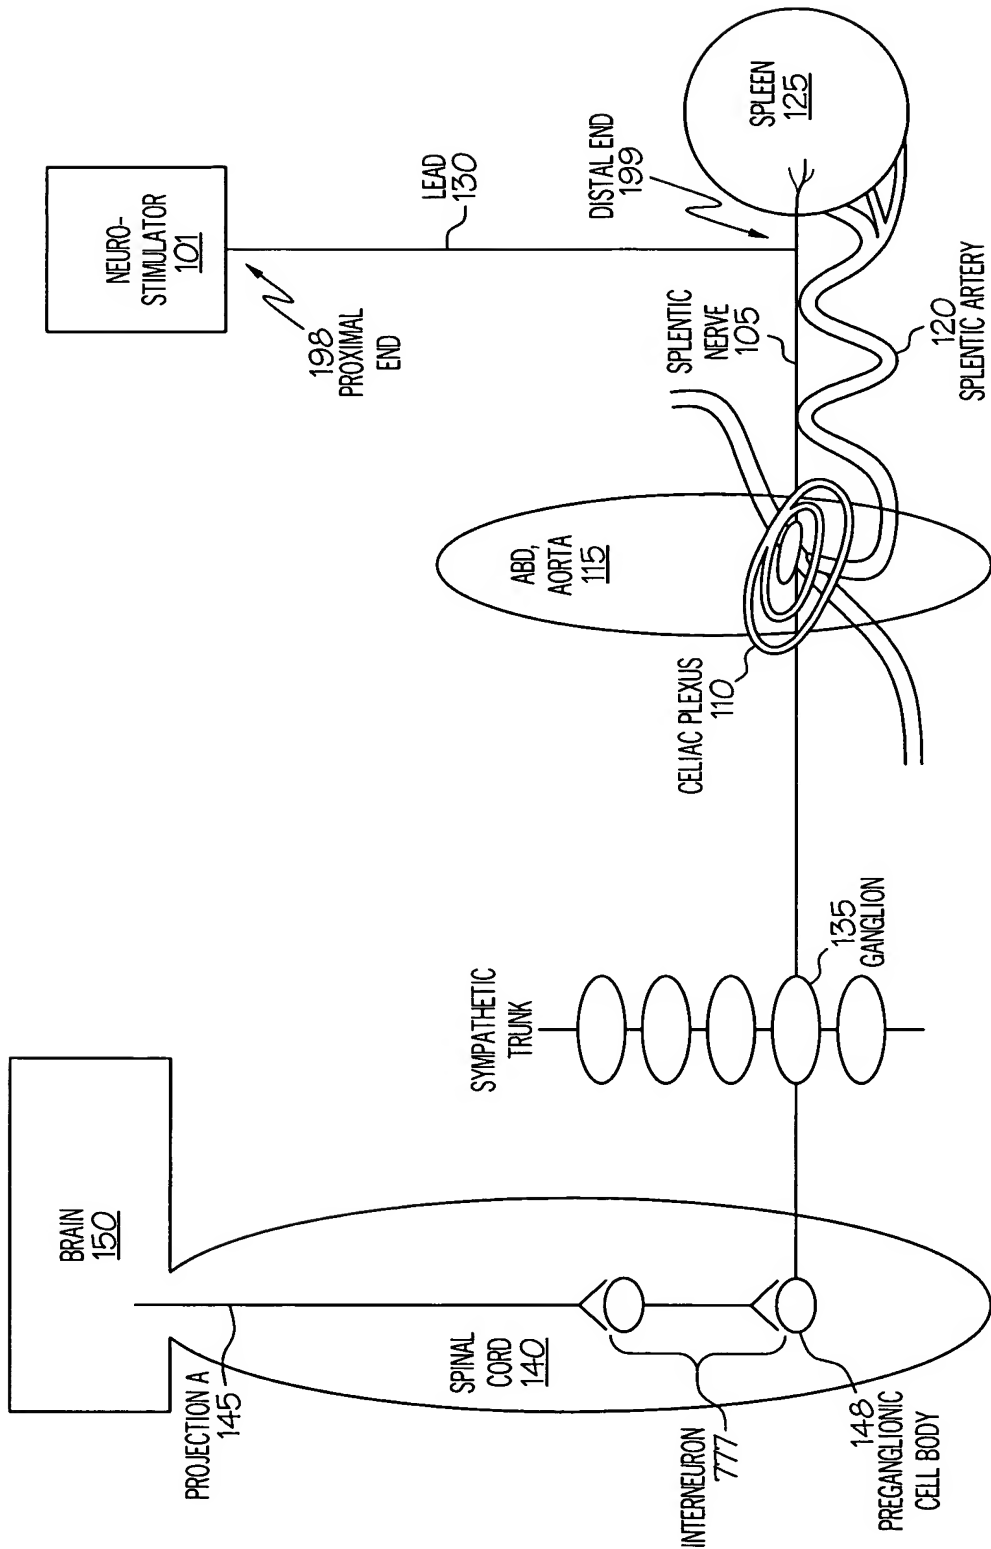


FIG. 9

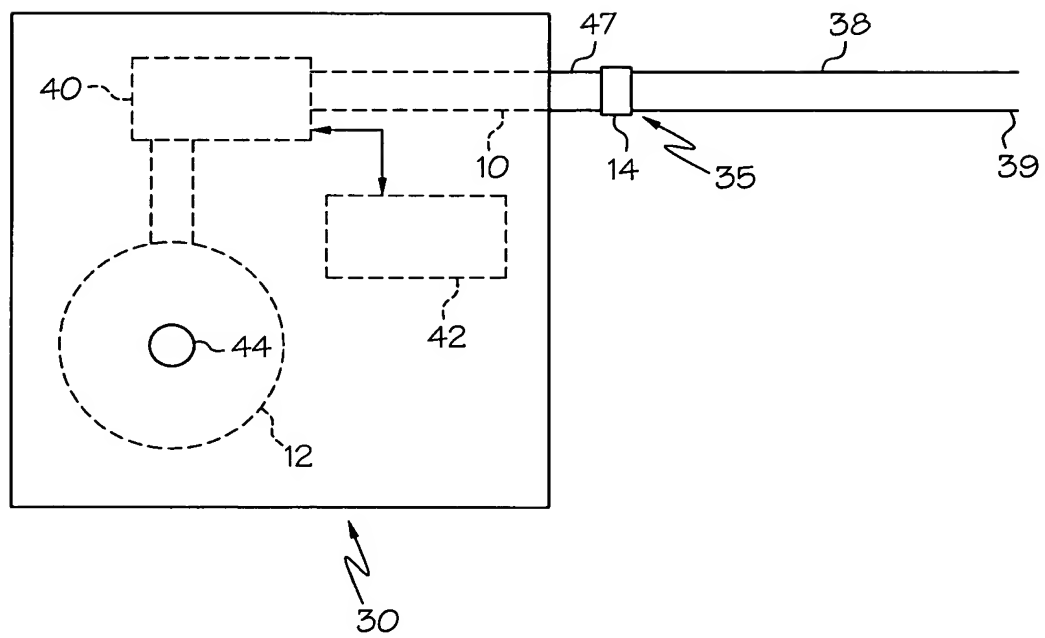


FIG. 10

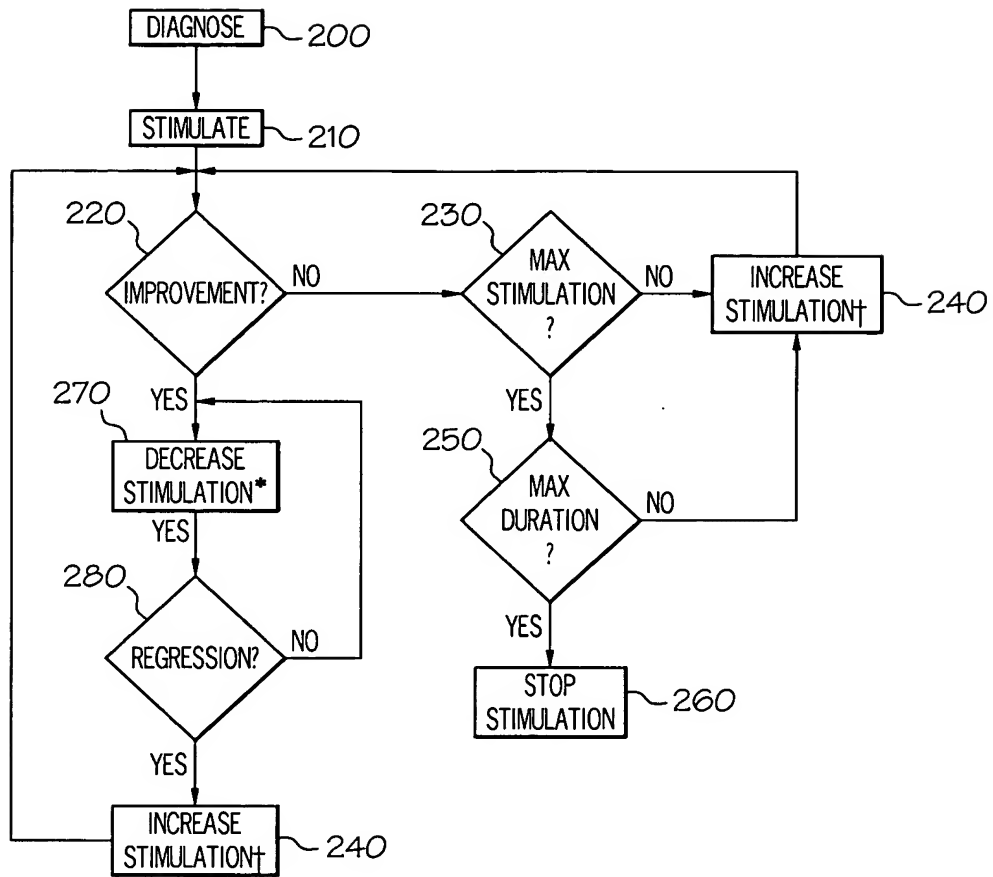


FIG. 11

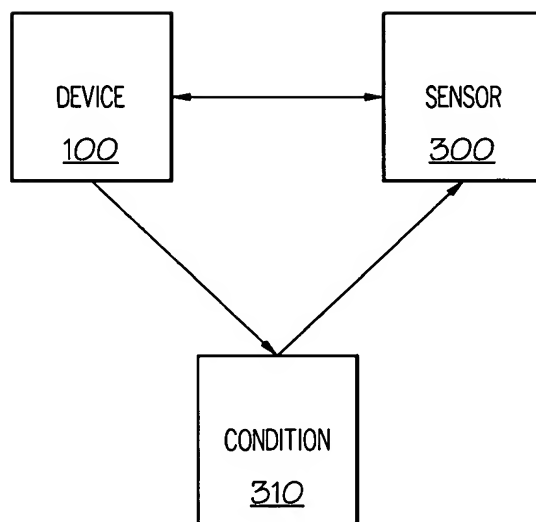


FIG. 12

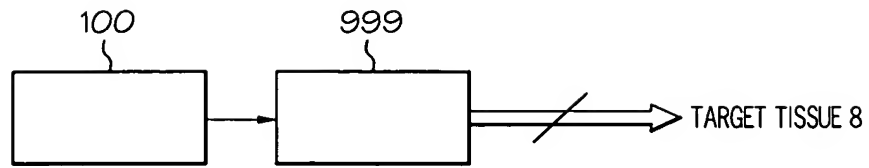


FIG. 13A

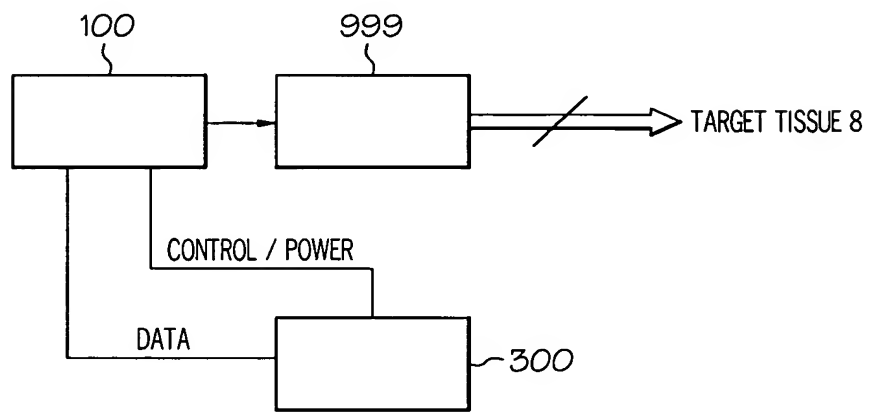


FIG. 13B

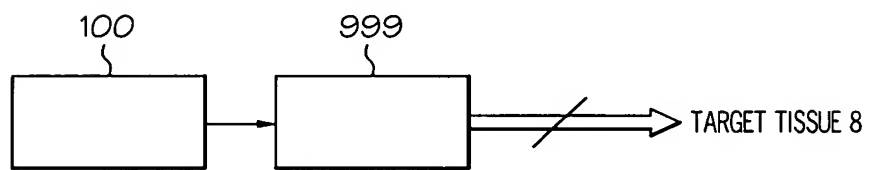


FIG. 13C

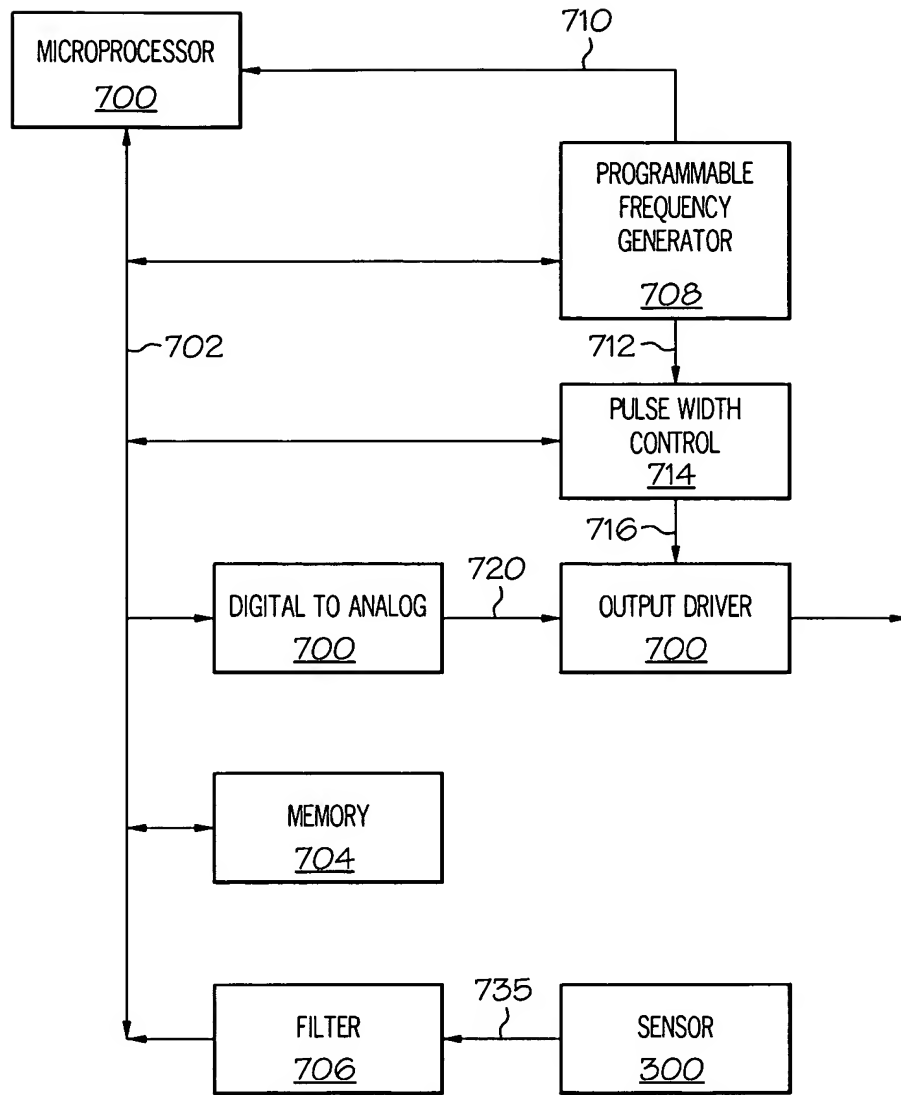


FIG. 14

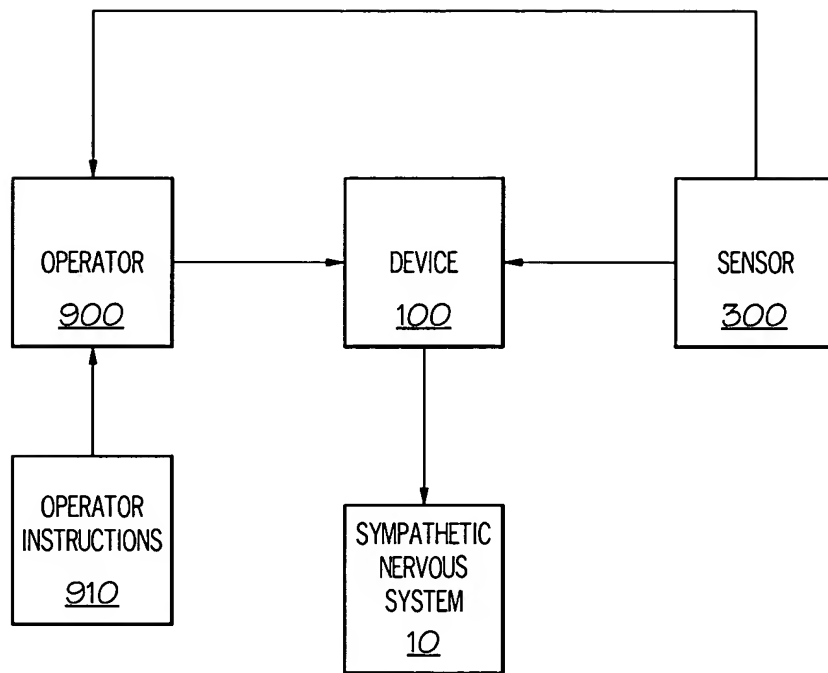


FIG. 15

18/26

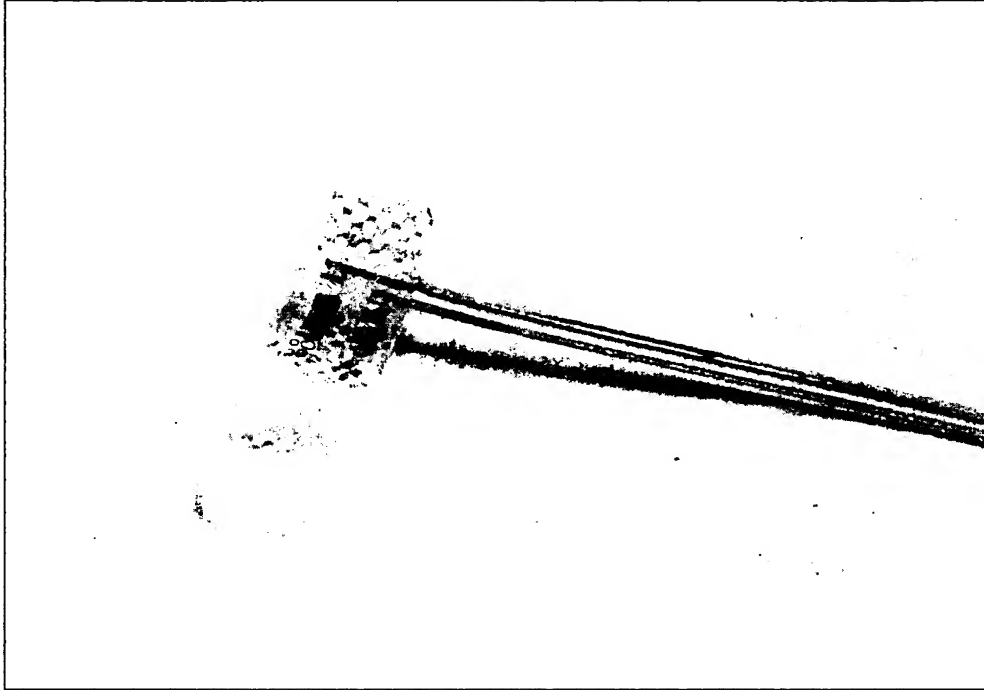


FIG. 16A

19/26

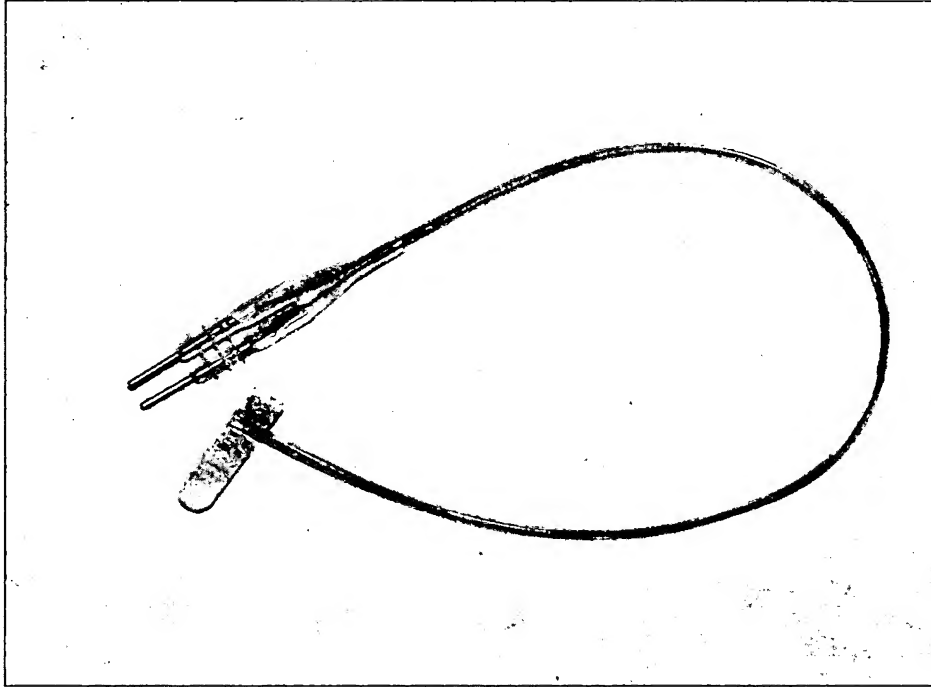


FIG. 16B

20/26



FIG. 17A

21/26



FIG. 17B

22/26



FIG. 17C

23/26

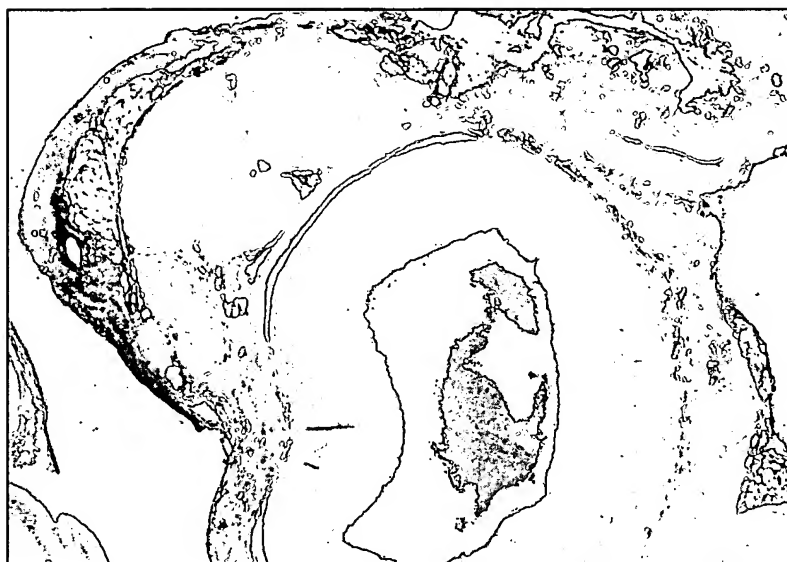


FIG. 17D

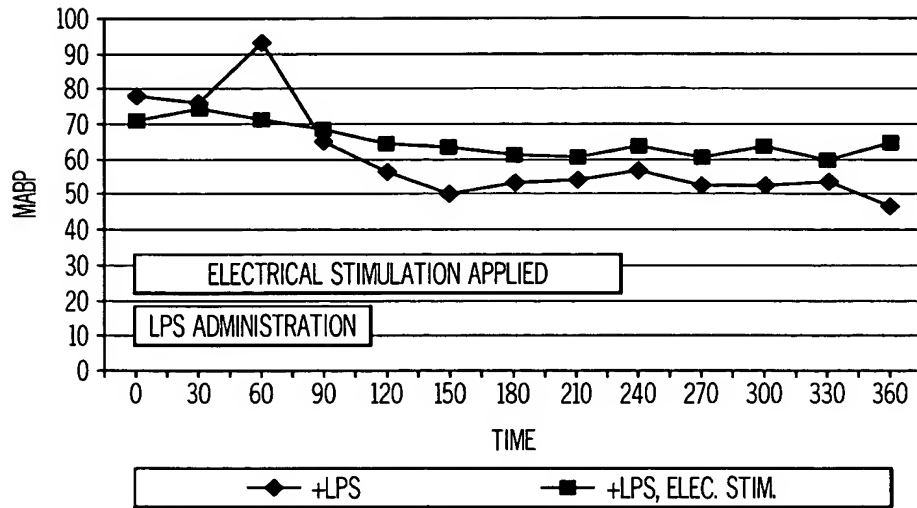


FIG. 18

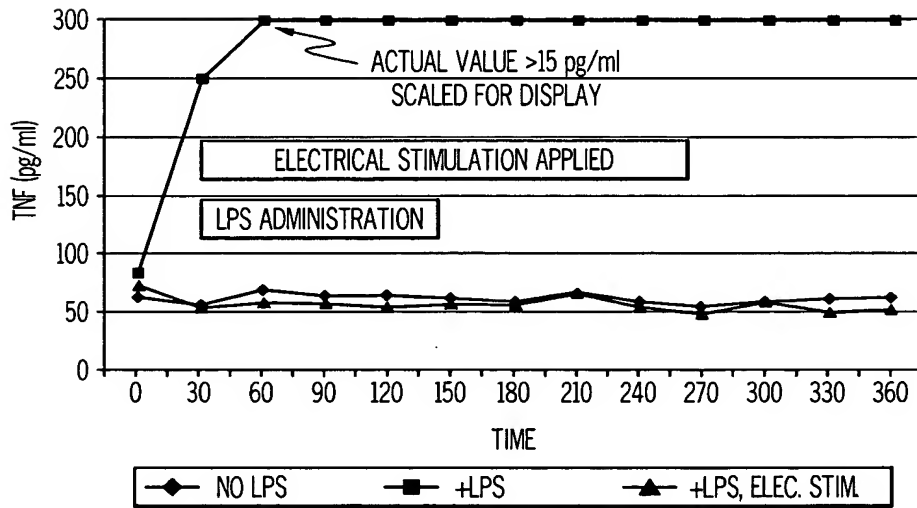


FIG. 19A

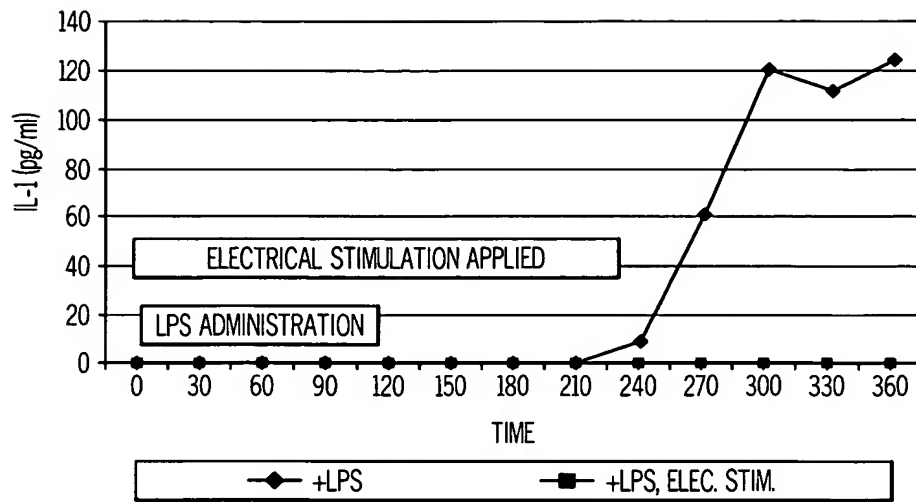


FIG. 19B

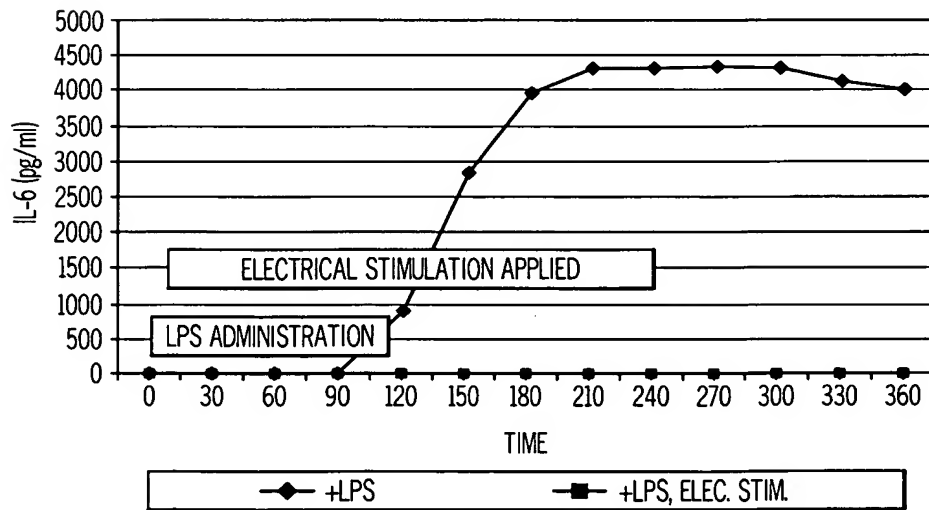


FIG. 19C

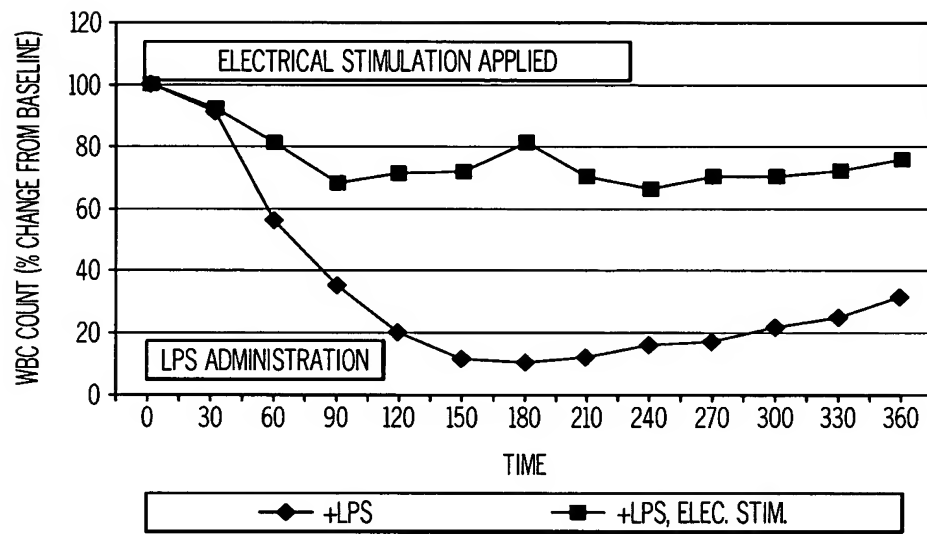


FIG. 20